

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **9032**

Date 02.02.2009


Expiry Date 30.01.2010

Reagent	Lot Number
AMM 1	9031
Amm 2	9032
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.022
0.25	Amm 10 09 08	0.222
0.50	Amm 10 09 08	0.431
0.77	Amm 10 09 08	0.651
1.00	Amm 10 09 08	0.842

**serial dilution*

Calibration Curve

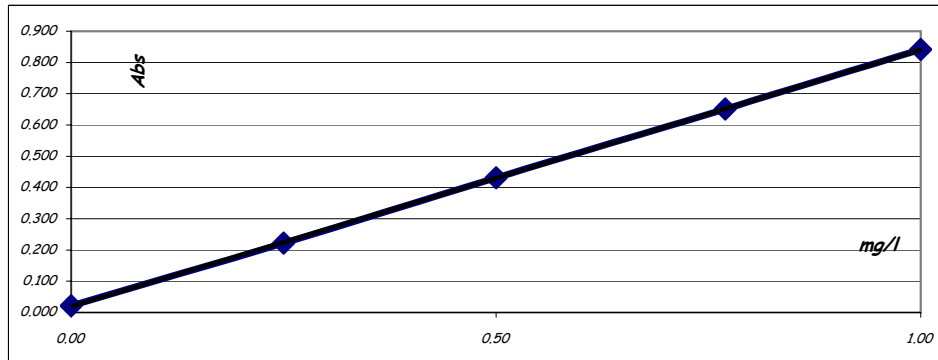

Test	Result	Specification	Pass / Fail
Intercept	0.0198	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8210	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*

**Stable on Board 5 days*

Barcode ID = 109

** Based on results obtained in our Research Facility*



Dr. T. Russell