

Certificate of Performance

Chloride Reagent


Product Code **KR101**
Lot Number **9046**

Date 11.03.2009 **Expiry Date** 03.03.2010

Reagent	Lot Number
Chloride	9046
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.002
250 ppm	cl4000 03 09	0.280
500 ppm	cl4000 03 09	0.452
800 ppm	cl4000 03 09	0.587
1000 ppm	cl4000 03 09	0.665

Calibration Curve

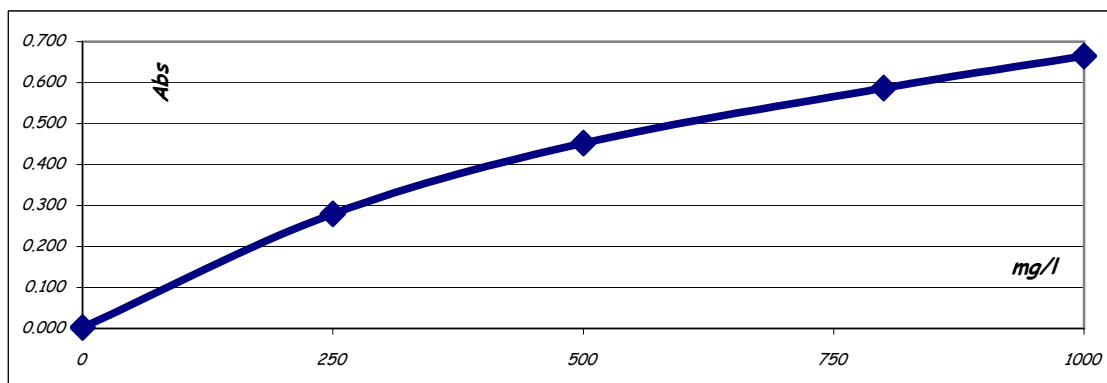

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0011	0.0010 to 0.0016	Pass
250 - 500 mg/l	0.0007	0.0006 to 0.0012	Pass
500 - 800 mg/l	0.0005	0.0004 to 0.0010	Pass
800 - 1000 mg/l	0.0004	0.0003 to 0.0008	Pass

Notes *Store between 2 & 8 °c*
 **Stable on Board 5 days*
 Barcode ID = 101
 ** Based on results obtained in our Research Facility*

Tom Russell.

Dr. T. Russell