

Certificate of Performance

Ammonia 1 Reagent

Product Code KR108
Lot Number 9052

Date 11.03.2009


Expiry Date 03.03.2010

Reagent	Lot Number
AMM 1	9052
Amm 2	9032
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.019
0.25	AMM 10 12 08	0.212
0.50	AMM 10 12 08	0.414
0.77	AMM 10 12 08	0.625
1.00	AMM 10 12 08	0.801

*serial dilution

Calibration Curve

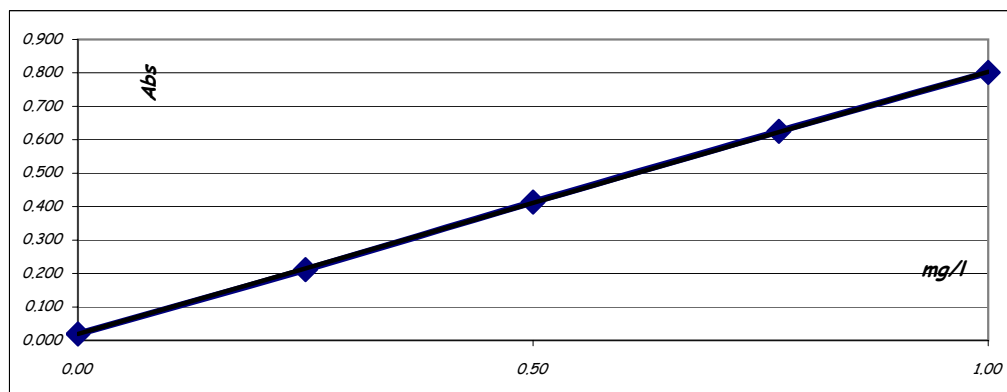

Test	Result	Specification	Pass / Fail
Intercept	0.0188	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7846	0.750 to 0.890	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes Store between 2 & 8 °c
 *Stable on Board 1 day
 Barcode ID = 108
 * Based on results obtained in our Research Facility

Tom Russell
 Dr. T. Russell