

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107  
Lot Number 9079

Date 08.04.2009


Expiry Date 02.04.2010

Reagent	Lot Number
Phos 1	9081
Phos 2	9079
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 01 09	0.147
1	P20 01 09	0.292
1.5	P20 01 09	0.450
2	P20 01 09	0.582

\*serial dilution

Calibration Curve

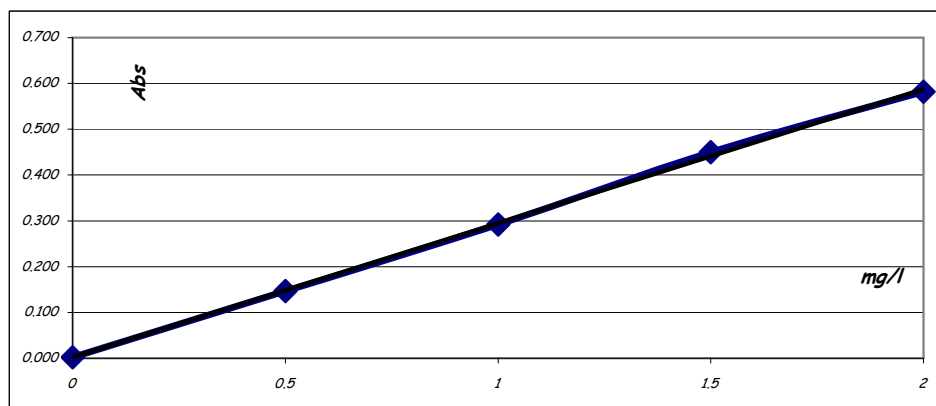

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.293	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C  
\*Stable on Board 5 days  
Barcode ID = 107  
\* Based on results obtained in our Research Facility

*Tom Russell.*  
Dr. T. Russell