Microgenics GmbH

'Ready To Use Reagents'

Certificate of Performance

Sulphate Reagent

Product Code KR102

Lot Number 0037

Date 02.03.2010 **Expiry Date** 25.02.2011

Reagent	Lot Number
Sulphate	0037
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #
0	
250	Sulp 4000 11 09
500	Sulp 4000 11 09
800	Sulp 4000 11 09
1000	Sulp 4000 11 09

*serial Dilution

Calibration Curve

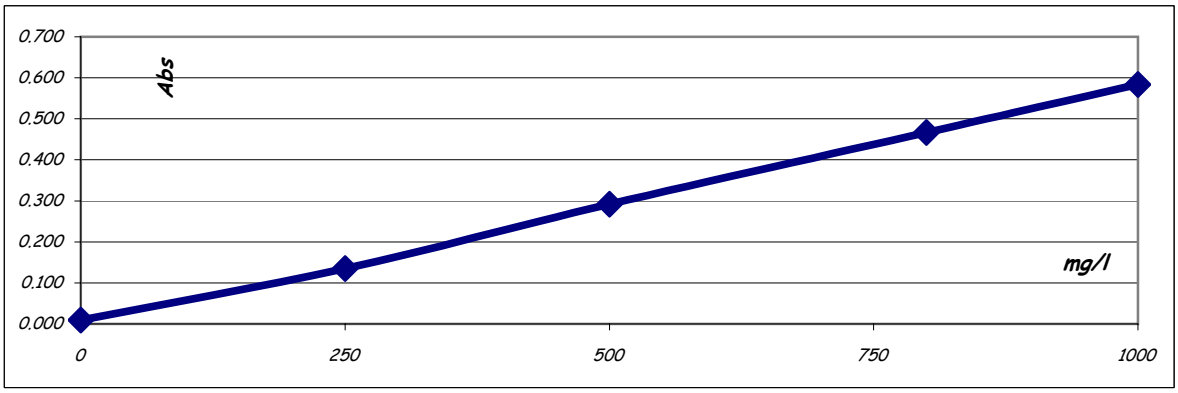

Test		Result	Specification			Pass / Fail
Intercept		0.009	-0.005	to	0.010	Pass
Sensitivity	Abs/ppm					
	0 - 250 mg/l	0.0005	0.0003	to	0.0006	Pass
	250 - 500 mg/l	0.0006	0.0003	to	0.0007	Pass
	500 - 800 mg/l	0.0006	0.0004	to	0.0007	Pass
	800 - 1000 mg/l	0.0006	0.0004	to	0.0008	Pass

Notes

Store between 2 & 8 °C

**Stable on Board 5 days*

Barcode ID = 102

** Based on results obtained in our Research Facility*

Tom Russell.

Dr. T. Russell

Telegraphic House, Waterfront Quay, Salford Quays, Manchester M50 3XW

Telephone 0161 869 0420

Microgenics GmbH