

**Certificate of Performance**
**TON 3**

Product Code KR105

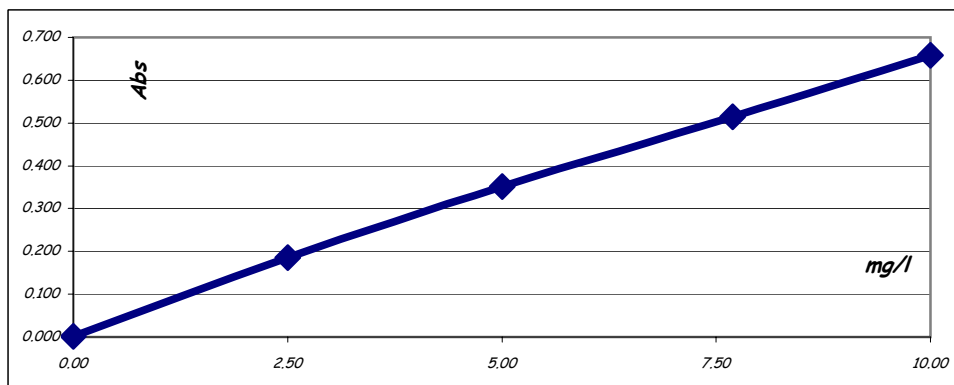
**Date** 26.02.2010

**Expiry Date** 25.02.2011

Reagent	Lot Number
TON 1	0038
TON 2	0040
TON 3	<b>0041</b>
<b>Test Method</b>	LMTP03
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.002
2.50	TON 100 11 09	0.186
5.00	TON 100 11 09	0.351
7.69	TON 100 11 09	0.515
10.00	TON 100 11 09	0.658

\*serial dilution

**Calibration Curve**


Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	<b>Pass</b>
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0736	0.0550 to 0.0800	<b>Pass</b>
2.50 - 5.00 mg/l	0.0660	0.0600 to 0.0800	<b>Pass</b>
5.00 - 7.69 mg/l	0.0610	0.0550 to 0.0800	<b>Pass</b>
7.69 - 10.0 mg/l	0.0619	0.0500 to 0.0700	<b>Pass</b>

**Notes** Store between 2 & 8 °C  
 \*Stable on Board TON 1 - 1 day  
     \* TON 2 & TON 3 - 5 days  
 Keep Tightly Sealed when not in use.  
 Do not return unused portions to container  
 Barcode ID- TON 1 103; TON 2 104; TON 3 105  
 \* Based on results obtained in our Research Facility



Dr. T. Russell