



Microgenics GmbH

'Ready To Use Reagents'

**Certificate of Performance**

**Phosphate 1 (Phos 1) Reagent**

**Product Code** KR106  
**Lot Number** 0070

**Date** 25.03.2010


**Expiry Date** 22.03.2011

Reagent	Lot Number
Phos 1	0070
Phos 2	9159
<b>Test Method</b>	LTP 05
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 01 10	0.137
1	P20 01 10	0.280
1.5	P20 01 10	0.432
2	P20 01 10	0.557

\*serial dilution

**Calibration Curve**

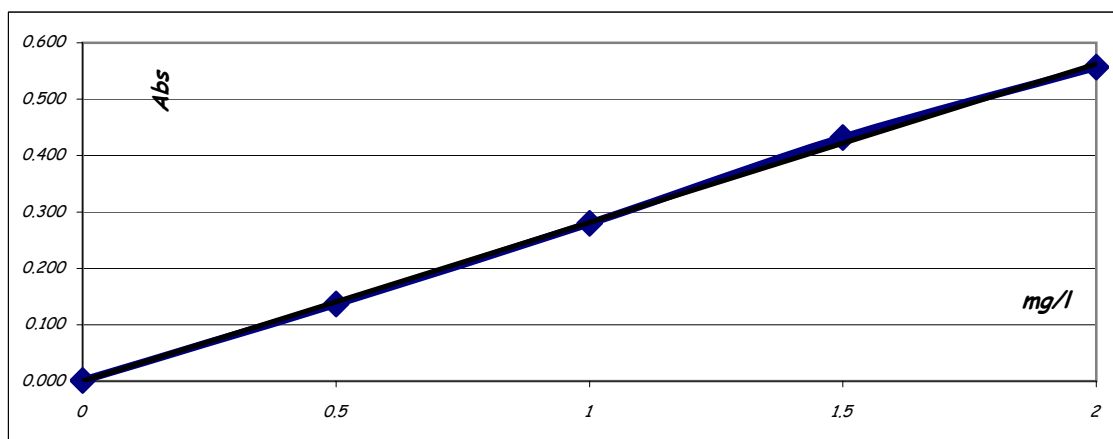

	Result	Specification	Pass / Fail
Intercept	0.000	-0.005 to 0.010	Pass
Sensitivity	Abs/ppm 0.281	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 106  
 \* Based on results obtained in our Research Facility

*Tom Russell.*

Dr. T. Russell