

## Certificate of Performance

### Ammonia 1 Reagent

**Product Code**      KR108  
**Lot Number**        0087

**Date**      22.04.2010


**Expiry Date**      21.04.2011

Reagent	Lot Number
AMM 1	0087
Amm 2	0086
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.018
0.25	AMM 10 03 10	0.222
0.50	AMM 10 03 10	0.433
0.77	AMM 10 03 10	0.655
1.00	AMM 10 03 10	0.851

*\*serial dilution*

### Calibration Curve

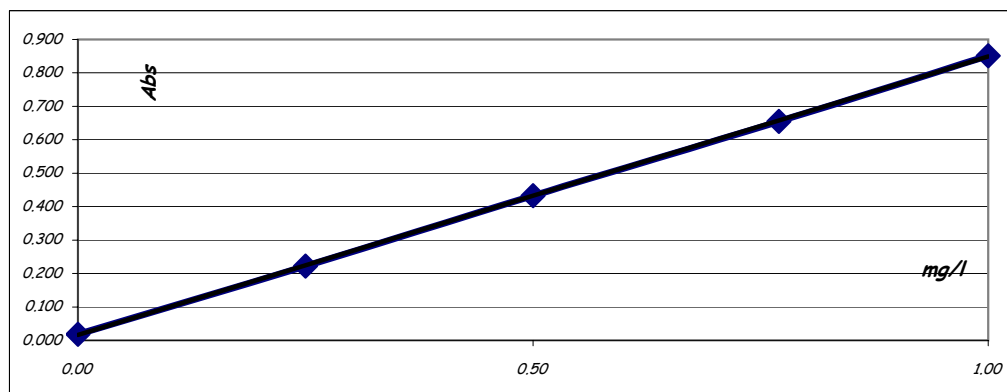

Test	Result	Specification	Pass / Fail
Intercept	0.0160	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8329	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

*Notes*      *Store between 2 & 8 °C*

*\*Stable on Board 1 day*

*Barcode ID = 108*

*\* Based on results obtained in our Research Facility*



*Dr. T. Russell*