



Microgenics GmbH

'Ready To Use Reagents'

**Certificate of Performance**

**Phosphate 1 (Phos 1) Reagent**

**Product Code**            **KR106**  
**Lot Number**                **0092**

**Date**                    26.04.2010


**Expiry Date**            21.04.2011

Reagent	Lot Number
Phos 1	0092
Phos 2	9228
<b>Test Method</b>	LTP 05
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.002
0.5	P20 03 10	0.151
1	P20 03 10	0.288
1.5	P20 03 10	0.438
2	P20 03 10	0.567

\*serial dilution

**Calibration Curve**

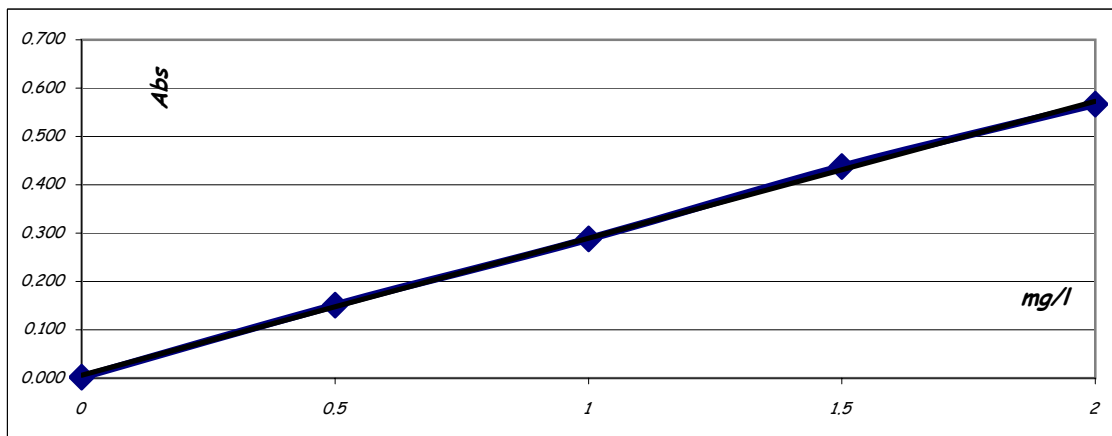

	Result	Specification	Pass / Fail
Intercept	0.006	-0.005 to 0.010	<b>Pass</b>
Sensitivity            Abs/ppm	0.283	0.260 to 0.320	<b>Pass</b>
Regression	0.999	0.990 to 1.001	<b>Pass</b>

**Notes**    Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 106  
 \* Based on results obtained in our Research Facility

*Tom Russell.*

Dr. T. Russell