

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **0109**

Date 27.05.2010


Expiry Date 26.05.2011

Reagent	Lot Number
AMM 1	0108
Amm 2	0109
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.024
0.25	Amm 10 03 10	0.225
0.50	Amm 10 03 10	0.432
0.77	Amm 10 03 10	0.656
1.00	Amm 10 03 10	0.857

**serial dilution*

Calibration Curve

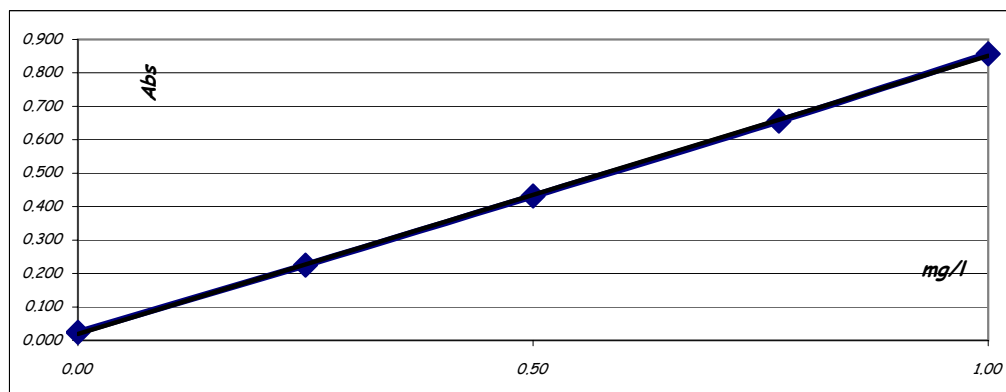

Test	Result	Specification	Pass / Fail
Intercept	0.0195	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8320	0.750 to 0.890	Pass
Regression	0.9998	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 109
** Based on results obtained in our Research Facility*



Dr. T. Russell