

Certificate of Performance
TON 2

Product Code KR104

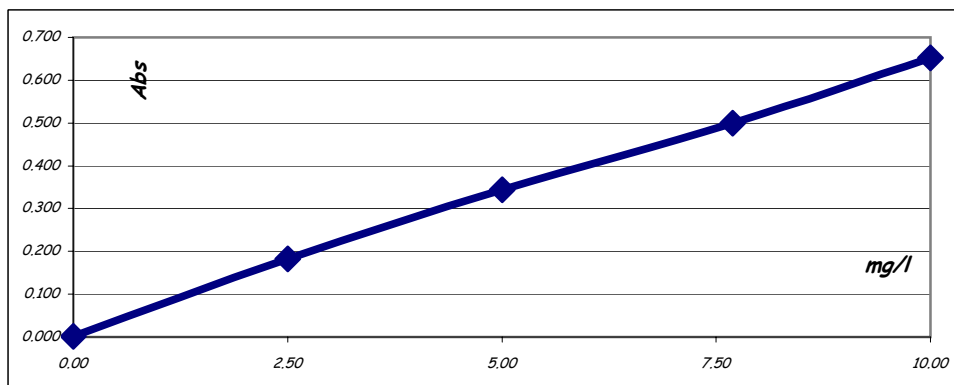
Date 01.06.2010

Expiry Date 26.05.2011

Reagent	Lot Number
TON 1	0021
TON 2	0110
TON 3	0111
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.002
2.50	TON 100 04 10	0.182
5.00	TON 100 04 10	0.344
7.69	TON 100 04 10	0.499
10.00	TON 100 04 10	0.652

*serial dilution

Calibration Curve


Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0720	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0648	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0576	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0662	0.0500 to 0.0700	Pass

Notes Store between 2 & 8 °C
 *Stable on Board TON 1 - 1 day
 * TON 2 & TON 3 - 5 days
 Keep Tightly Sealed when not in use.
 Do not return unused portions to container
 Barcode ID- TON 1 103; TON 2 104; TON 3 105
 * Based on results obtained in our Research Facility



Dr. T. Russell