

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **0153**

Date 29.07.2010


Expiry Date 27.07.2011

Reagent	Lot Number
AMM 1	0152
Amm 2	0153
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.030
0.25	Amm 10 06 10	0.202
0.50	Amm 10 06 10	0.395
0.77	Amm 10 06 10	0.599
1.00	Amm 10 06 10	0.780

**serial dilution*

Calibration Curve

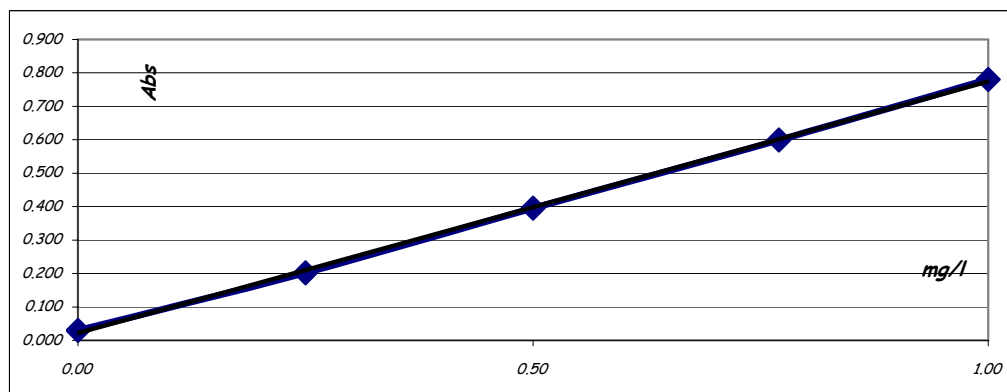

Test	Result	Specification	Pass / Fail
Intercept	0.0218	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7527	0.750 to 0.890	Pass
Regression	0.9995	0.990 to 1.0001	Pass

Notes

Store between 2 & 8 °c

**Stable on Board 5 days*

Barcode ID = 109

** Based on results obtained in our Research Facility*



Dr. T. Russell