



Microgenics GmbH

'Ready To Use Reagents'

Certificate of Performance

Sulphate Reagent

Product Code **KR102**
Lot Number **0154**


Date 30.07.2010 **Expiry Date** 27.07.2011

Reagent	Lot Number
Sulphate	0154
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #
0	
250	Sulp 4000 05 10
500	Sulp 4000 05 10
800	Sulp 4000 05 10
1000	Sulp 4000 05 10

*serial Dilution

Calibration Curve

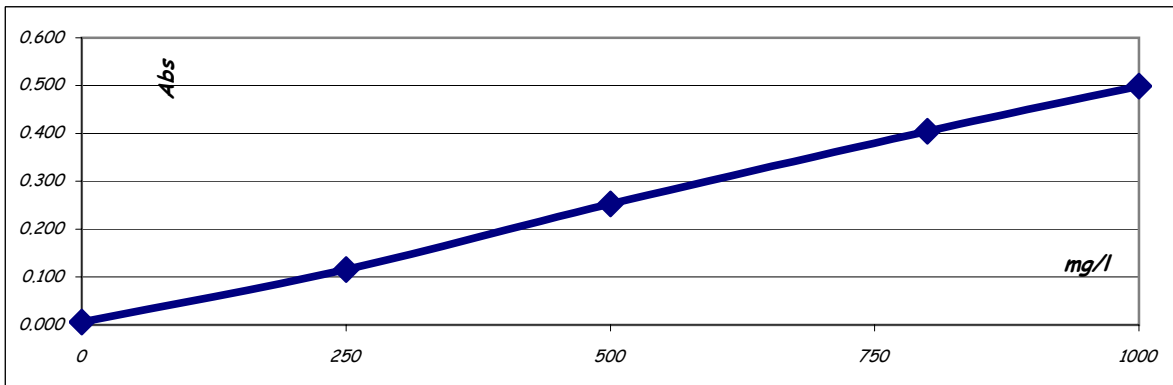

Test	Result	Specification	Pass / Fail	
Intercept	0.006	-0.005 to 0.010	Pass	
Sensitivity	Abs/ppm			
	0 - 250 mg/l	0.0004	0.0003 to 0.0006	Pass
	250 - 500 mg/l	0.0005	0.0003 to 0.0007	Pass
	500 - 800 mg/l	0.0005	0.0004 to 0.0007	Pass
	800 - 1000 mg/l	0.0005	0.0004 to 0.0008	Pass

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 102
** Based on results obtained in our Research Facility*

Tom Russell.

Dr. T. Russell

Telegraphic House, Waterfront Quay, Salford Quays, Manchester M50 3XW

Microgenics GmbH

Telephone 0161 869 0420