



Microgenics GmbH

'Ready To Use Reagents'

Certificate of Performance

Sulphate Reagent

Product Code **KR102**
Lot Number **0183**


Date 27.09.2010 **Expiry Date** 23.09.2011

Reagent		Lot Number	
Sulphate	0183		
Test Method		LTP01	
Test Instrument		Konelab 20	
Serial Number		P4919028	

Standard Value	Lot #
0	
250	Sulp 4000 05 10
500	Sulp 4000 05 10
800	Sulp 4000 05 10
1000	Sulp 4000 05 10

*serial Dilution

Calibration Curve

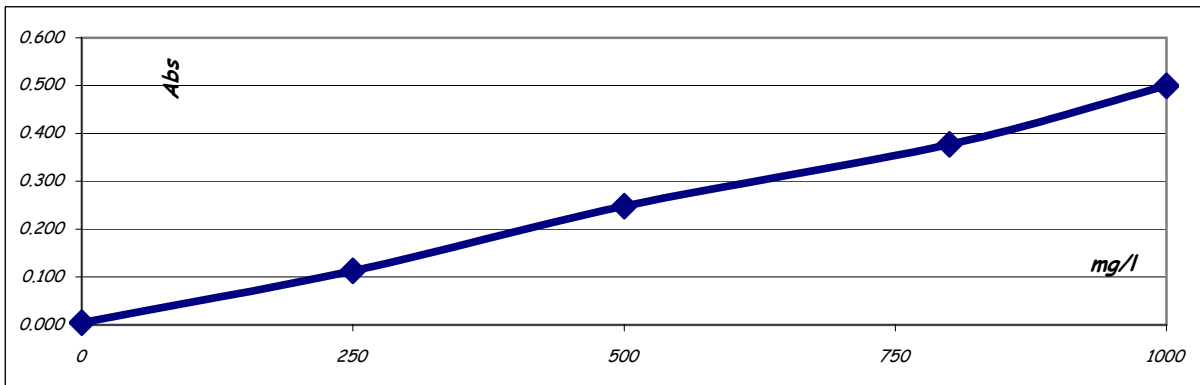

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to	Pass
Sensitivity	Abs/ppm		
	0 - 250 mg/l	0.0004 to 0.0003	Pass
	250 - 500 mg/l	0.0005 to 0.0003	Pass
	500 - 800 mg/l	0.0004 to 0.0004	Pass
800 - 1000 mg/l	0.0006 to 0.0004	Pass	

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 102
** Based on results obtained in our Research Facility*

Tom Russell.

Dr. T. Russell

Telegraphic House, Waterfront Quay, Salford Quays, Manchester M50 3XW

Microgenics GmbH

Telephone 0161 869 0420