

## Certificate of Performance

### Sulphate Reagent

**Product Code** KR102

**Lot Number** 0190

**Date** 18.10.2010


**Expiry Date** 12.10.2011

<b>Reagent</b>	<b>Lot Number</b>
Sulphate	0190
<b>Test Method</b>	LTP01
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.004
250	Sulp 4000 05 10	0.109
500	Sulp 4000 05 10	0.238
800	Sulp 4000 05 10	0.395
1000	Sulp 4000 05 10	0.491

\*serial Dilution

### Calibration Curve

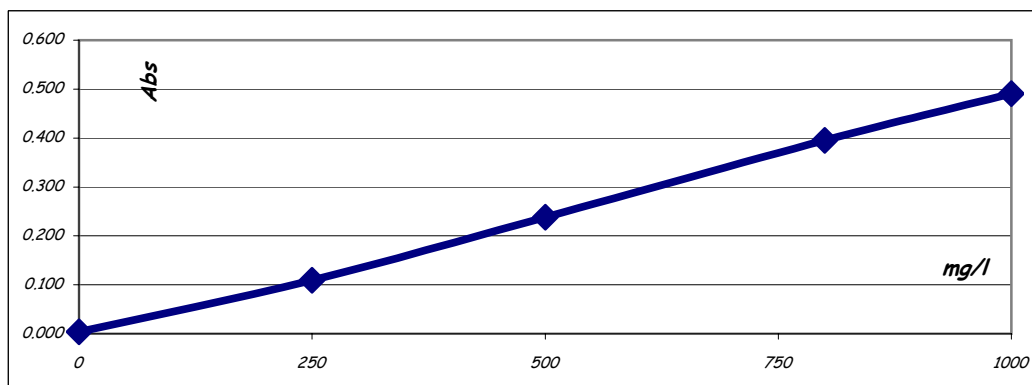

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	<b>Pass</b>
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0004	0.0003 to 0.0005	<b>Pass</b>
250 - 500 mg/l	0.0005	0.0003 to 0.0006	<b>Pass</b>
500 - 800 mg/l	0.0005	0.0004 to 0.0007	<b>Pass</b>
800 - 1000 mg/l	0.0005	0.0004 to 0.0008	<b>Pass</b>

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 102  
 \* Based on results obtained in our Research Facility



*Dr. T. Russell*