



Microgenics GmbH

'Ready To Use Reagents'

Certificate of Performance

Phosphate 1 (Phos 1) Reagent

Product Code **KR106**
Lot Number **0191**

Date 14.10.2010


Expiry Date 12.10.2011

Reagent	Lot Number
Phos 1	0191
Phos 2	9228
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 09 10	0.154
1	P20 09 10	0.295
1.5	P20 09 10	0.446
2	P20 09 10	0.587

*serial dilution

Calibration Curve

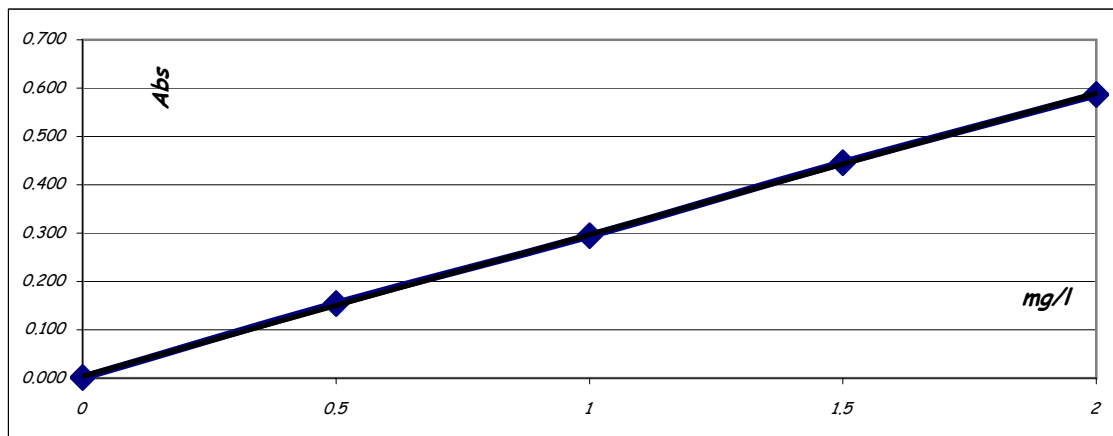

	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.010	Pass
Sensitivity	Abs/ppm 0.293	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 106
 * Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell