

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      KR 109  
**Lot Number**        0221

**Date**            15.11.2010


**Expiry Date**    10.11.2011

Reagent	Lot Number
AMM 1	0220
Amm 2	<b>0221</b>
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.019
0.25	Amm 10 07 10	0.234
0.50	Amm 10 07 10	0.441
0.77	Amm 10 07 10	0.671
1.00	Amm 10 07 10	0.879

*\*serial dilution*

#### Calibration Curve

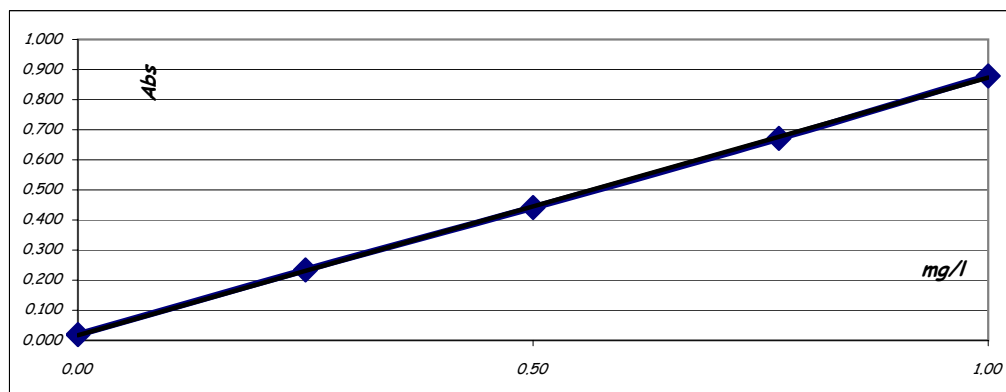

Test	Result	Specification	Pass / Fail
Intercept	0.0175	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8558	0.750 to 0.890	<b>Pass</b>
Regression	0.9998	0.990 to 1.0001	<b>Pass</b>

**Notes**    *Store between 2 & 8 °c*  
*\*Stable on Board 5 days*  
*Barcode ID = 109*  
*\* Based on results obtained in our Research Facility*


---

 Dr. T. Russell