



Microgenics GmbH

Ready To Use Reagents'

Certificate of Performance

Phosphate 1 (Phos 1) Reagent

Product Code KR106
Lot Number 0267

Date 07.12.2010


Expiry Date 01.12.2011

Reagent	Lot Number
Phos 1	0267
Phos 2	0268
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.003
0.5	P20 06 10	0.146
1	P20 06 10	0.289
1.5	P20 06 10	0.446
2	P20 06 10	0.579

*serial dilution

Calibration Curve

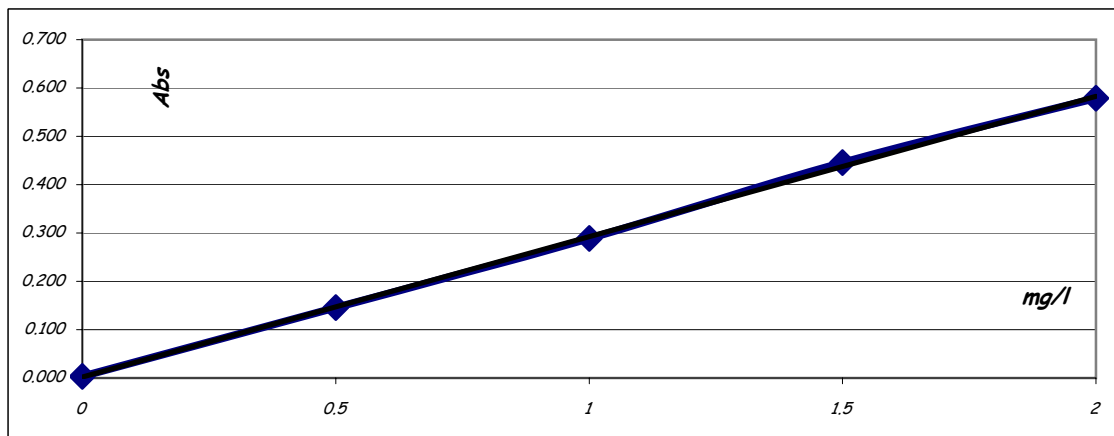

	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity	Abs/ppm 0.290	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 106
 * Based on results obtained in our Research Facility

Dr. T. Russell