



Microgenics GmbH

'Ready To Use Reagents'

**Certificate of Performance**

**Phosphate 2 (Phos 2) Reagent**

**Product Code** KR107  
**Lot Number** 0268

**Date** 07.12.2010


**Expiry Date** 01.12.2011

Reagent	Lot Number
Phos 1	0267
Phos 2	0268
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.003
0.5	P20 06 10	0.146
1	P20 06 10	0.289
1.5	P20 06 10	0.446
2	P20 06 10	0.579

\*serial dilution

**Calibration Curve**

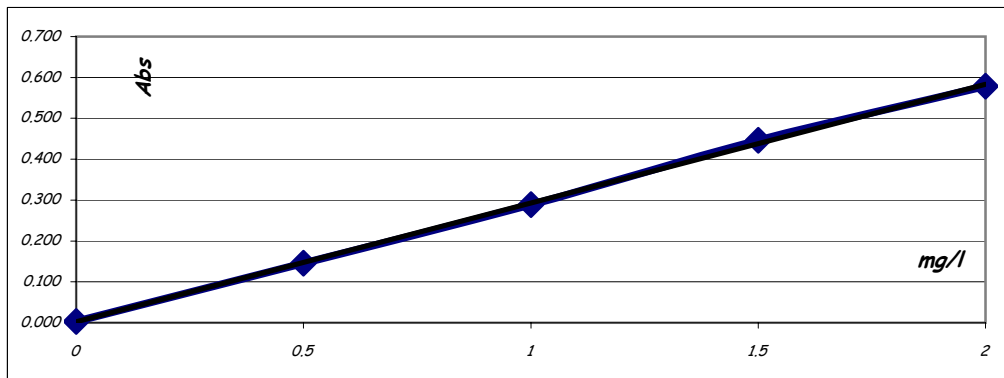

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.290	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility

*Tom Russell.*  
 Dr. T. Russell