

Certificate of Performance

Ammonia 2 Reagent

Product Code KR 109
Lot Number 0270

Date 13.12.2010


Expiry Date 01.12.2011

Reagent	Lot Number
AMM 1	0269
Amm 2	0270
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.020
0.25	Amm 10 07 10	0.228
0.50	Amm 10 07 10	0.436
0.77	Amm 10 07 10	0.656
1.00	Amm 10 07 10	0.859

**serial dilution*

Calibration Curve

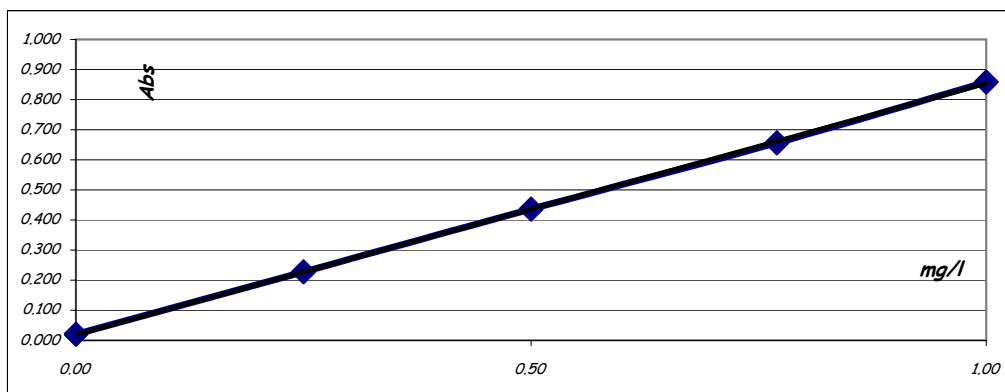

Test	Result	Specification	Pass / Fail
Intercept	0.0187	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8355	0.750 to 0.890	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes Store between 2 & 8 °c
 *Stable on Board 5 days
 Barcode ID = 109
 * Based on results obtained in our Research Facility

Tom Russell

 Dr. T. Russell