

Certificate of Performance

TON 2 Reagent

Product Code **KR 104**
 Lot Number **4059**


Date **07.09.2004**

Expiry Date **04.03.2005**

Reagent	Lot Number
TON 1	4057
TON 2	4059
TON 3	4061
Test Method	LMTPO3
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.006
2.5	TON2.5 210 04	0.173
5	TON5.0 210 04	0.343
7.5	TON7.5 210 04	0.501
10	TON10 210 04	0.638

Calibration Curve

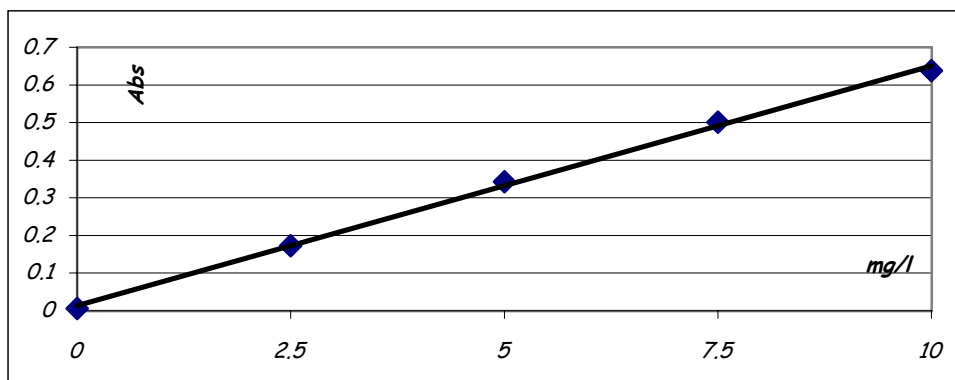

Test	Result	Specification	Pass / Fail
Intercept	0.006	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.5 mg/l	0.0069	0.0055 to 0.0080	Pass
2.5 - 5.0 mg/l	0.0068	0.0060 to 0.0080	Pass
5.0 - 7.5 mg/l	0.0063	0.0050 to 0.0075	Pass
7.5 - 10.0 mg/l	0.0055	0.0050 to 0.0070	Pass

Tom Russell

Dr. T. Russell