

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107
 Lot Number 4092


Date 01.11.2004

Expiry Date 01.05.2005

Reagent	Lot Number
Phos 1	4091
Phos 2	4092
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0
0.5	P0.5 279 04	0.151
1	P1.0 278 04	0.301
1.5	P1.5 279 04	0.453
2	P2.0 279 04	0.596

Calibration Curve

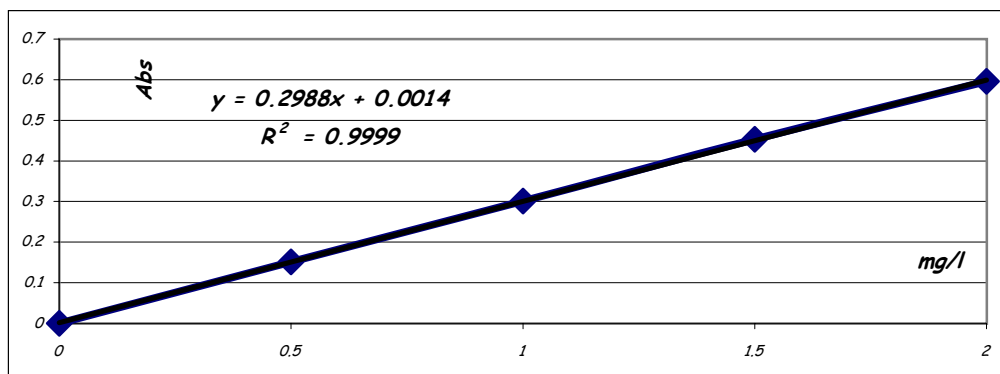

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.010	Pass
Sensitivity	Abs/ppm 0.299	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass



Dr. T. Russell