

## Certificate of Performance

### TON 2 Reagent

**Product Code**                      **KR 104**  
**Lot Number**                         **4094**


**Date**            01.11.2004

**Expiry Date**            02.05.2005

Reagent	Lot Number
TON 1	4093
TON 2	<b>4094</b>
TON 3	4095
<b>Test Method</b>	LMTPO3
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0		0.006
2.5	TON2.5 272 04	0.171
5	TON5.0 272 04	0.339
7.5	TON7.5 272 04	0.494
10	TON10 272 04	0.665

### Calibration Curve

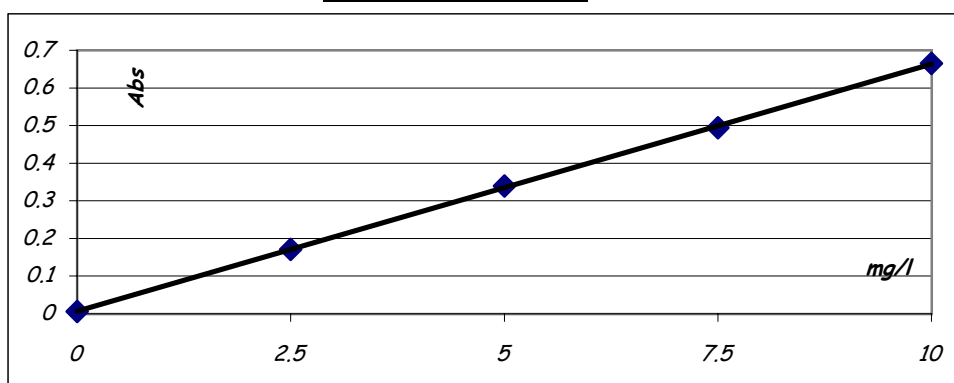

Test	Result	Specification	Pass / Fail
Intercept	0.006	-0.005 to 0.01	<b>Pass</b>
Sensitivity			
Abs/ppm			
0 - 2.5 mg/l	0.0068	0.0055 to 0.0080	<b>Pass</b>
2.5 - 5.0 mg/l	0.0067	0.0060 to 0.0080	<b>Pass</b>
5.0 - 7.5 mg/l	0.0062	0.0050 to 0.0075	<b>Pass</b>
7.5 - 10.0 mg/l	0.0068	0.0050 to 0.0070	<b>Pass</b>

*Tom Russell.*

\_\_\_\_\_  
Dr. T. Russell