

Certificate of Performance

Phos 1 Reagent



Product Code 984644

984646

Lot Number 0010

Date 08 .01.2010


Expiry Date 04.01.2011

Reagent	Lot Number
Phos 1	0010
Phos 2	0009
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 08 09	0.140
1	P20 08 09	0.285
1.5	P20 08 09	0.431
2	P20 08 09	0.560

*serial dilution

Calibration Curve

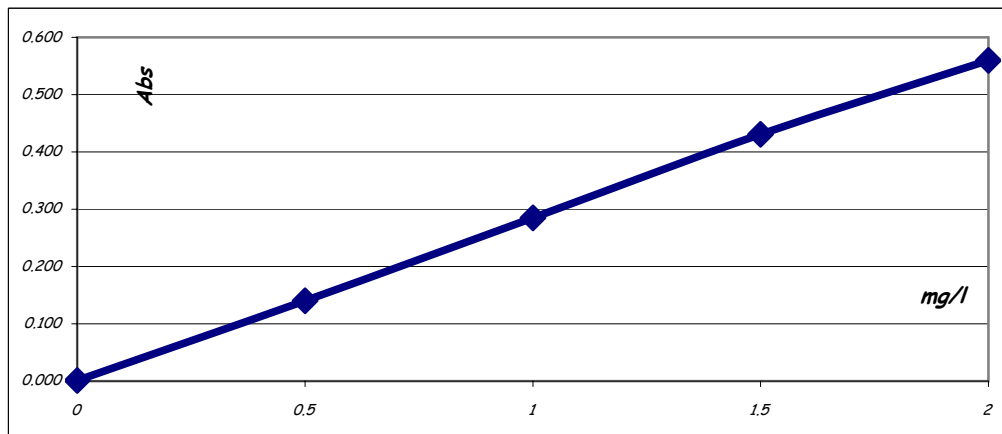

	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.282	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
*Stable on Board 5 days
Barcode ID = 763
* Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell